



SOUTH CHINA NATIONAL CENTER OF METROLOGY
GUANGDONG INSTITUTE OF METROLOGY

TEST REPORT

No. XNZ202502070

Name of Sample: Power Quality Analyzer

Model / Type: APView400
230 V 5A 50/60Hz

Sample Number: 02125022200003

Applicant: Acrel Co., Ltd.

Manufacturer: Jiangsu Acrel Electrical Manufacturing Co., Ltd.

Test Type: Commission

Date Issued: 2025-04-23



DIRECTIONS

1. This report shall not be reproduced except in full, or extracted, without the written approval of our laboratory.
2. Testing results provided by this report relate only to the samples tested.
3. This report shall not be valid if smeared or altered.
4. This report shall not be valid without stamp.
5. Complaint shall be raised to the report-issuing department within 15 days upon receipt of the report on which the applicant casts doubt. No complaint shall be accepted after deadline.

Headquarter Address: No.30, Songbai East Street, Guangyuan Middle Road,
GuangZhou, Guangdong,China

Dongguan Branch Address: No.152, Shipai Duan, Dongyuan Road, Shipai
Town, Dongguan, Guangdong, China

Tel. : (8620) 26297181


Fax: (8620) 26297181

E-mail: zl@scm.com.cn

Website: <http://www.scm.com.cn>

(1) Basic Information

Name of Sample	Power Quality Analyzer	Trade Mark	--
Model / Type	APView400 230 V 5 A 50/60 Hz	Class	Class A
Sample No.	02125022200003	Sample quantity	1
Applicant	Acrel Co., Ltd.		
Address	No. 253, Yulv Road, Jiading, Shanghai, China		
Manufacturer	Jiangsu Acrel Electrical Manufacturing Co., Ltd.		
Test Site	Environment and EMC Lab of Dongguan Branch		
Test Conditions	Temperature: (20±3) °C Humidity: (45~60)%RH		
Date Received	Mar. 6, 2025	Commission No.	WT20252096
Test Date	Apr. 21, 2025 to Apr. 23, 2025	Test Type	Commission
Test Item	See "Test Results Summary"		
Test Standard	<ol style="list-style-type: none"> 1. The applicant's test requirements 2. IEC 61000-4-30 (Edition 3.1): 2021 Electromagnetic compatibility(EMC) – Part 4-30 : Testing and measurement techniques – Power quality measurement methods 3. IEC 62586-2(Edition 2.1): 2021 Power quality measurement in power supply systems – Part 2 : Functional tests and uncertainty requirements 		
Conclusion	PASS	(Seal of Report)	
Remarks	This report is for scientific research and internal quality control use only.		

Tested by: 

Checked by:  Approved by: 

(2) Test Results Summary


No.	Test Item	Test Standard	Sample No.	Pass (P)	Fail (F)
1	Power frequency	IEC 61000-4-30 (Edition 3.1) : 2021 IEC 62586-2 (Edition2.1) : 2021	021250222000 03	P	
2	Magnitude of supply voltage	IEC 61000-4-30 (Edition 3.1) : 2021 IEC 62586-2 (Edition2.1) : 2021	021250222000 03	P	
3	Flicker	IEC 61000-4-30 (Edition 3.1) : 2021 IEC 62586-2 (Edition2.1) : 2021	021250222000 03	P	
4	Supply voltage interruptions, dips and swells	IEC 61000-4-30 (Edition 3.1) : 2021 IEC 62586-2 (Edition2.1) : 2021	021250222000 03	P	
5	Supply voltage unbalance	IEC 61000-4-30 (Edition 3.1) : 2021 IEC 62586-2 (Edition2.1) : 2021	021250222000 03	P	
6	Voltage harmonics	IEC 61000-4-30 (Edition 3.1) : 2021 IEC 62586-2 (Edition2.1) : 2021	021250222000 03	P	
7	Voltage interharmonics	IEC 61000-4-30 (Edition 3.1) : 2021 IEC 62586-2 (Edition2.1) : 2021	021250222000 03	P	
8	Mains signalling voltages on the supply voltage	IEC 61000-4-30 (Edition 3.1) : 2021 IEC 62586-2 (Edition2.1) : 2021	021250222000 03	P	
9	Measurement of underdeviation and overdeviation parameters	IEC 61000-4-30 (Edition 3.1) : 2021 IEC 62586-2 (Edition2.1) : 2021	021250222000 03	P	

No.	Test Item	Test Standard	Sample No.	Pass (P)	Fail (F)
10	Flagging	IEC 61000-4-30 (Edition 3.1) : 2021 IEC 62586-2 (Edition2.1) : 2021	021250222000 03	P	
11	Variations due to external influence quantities	IEC 61000-4-30 (Edition 3.1) : 2021 IEC 62586-2 (Edition2.1) : 2021	021250222000 03	P	
12	Rapid voltage changes (RVC)	IEC 61000-4-30 (Edition 3.1) : 2021 IEC 62586-2 (Edition2.1) : 2021	021250222000 03	P	
13	Magnitude of current	IEC 61000-4-30 (Edition 3.1) : 2021 IEC 62586-2 (Edition2.1) : 2021	021250222000 03	P	
14	Harmonic current	IEC 61000-4-30 (Edition 3.1) : 2021 IEC 62586-2 (Edition2.1) : 2021	021250222000 03	P	
15	Interharmonic currents	IEC 61000-4-30 (Edition 3.1) : 2021 IEC 62586-2 (Edition2.1) : 2021	021250222000 03	P	
16	Current unbalance	IEC 61000-4-30 (Edition 3.1) : 2021 IEC 62586-2 (Edition2.1) : 2021	021250222000 03	P	
17	Calculation of measurement uncertainty and operating uncertainty	IEC 61000-4-30 (Edition 3.1) : 2021 IEC 62586-2 (Edition2.1) : 2021	021250222000 03	P	

(3) Sample Photo



Picture of sample appearance

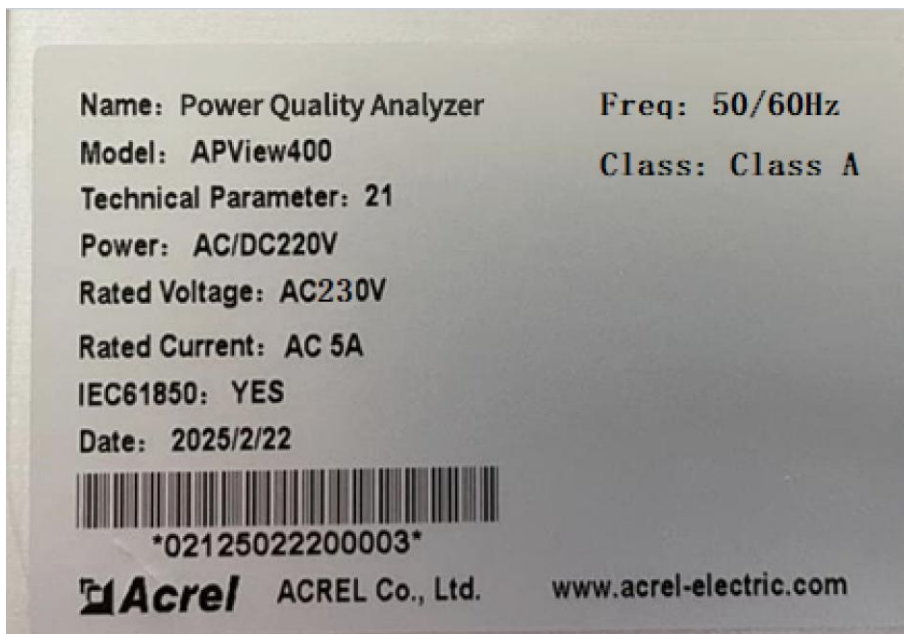

Picture of sample nameplates

ANNEX A

Table 1 – Testing points for each measured parameter

Measured parameter	Class	Testing point P1	Testing point P2	Testing point P3	Testing point P4	Testing point P5
Frequency 50 Hz (covers 50 Hz)	A or S	42,5 Hz	50,05 Hz	57,5 Hz	50 Hz	N.A.
Frequency 60 Hz (covers 60 Hz)	A or S	51 Hz	59,95 Hz	69Hz	60 Hz	N.A.
Voltage magnitude	A	10% U_{din}	45% U_{din}	80% U_{din}	115% U_{din}	150% U_{din}
	S	20% U_{din}	45% U_{din}	70% U_{din}	95% U_{din}	120% U_{din}
Magnitude of current	A or S	10% I_n	45% I_n	80% I_n	100% I_n	N.A.
Swells	A	Threshold swell –	Threshold swell +	110% U_{din}	120% U_{din}	200% U_{din}
	S	Threshold swell –	Threshold swell +	110% U_{din}	120% U_{din}	150% U_{din}
Dips	A	Threshold dip–	Threshold dip+	20% U_{din}	60% U_{din}	85% U_{din}
	S	Threshold dip–	Threshold dip+	20% U_{din}	60% U_{din}	85% U_{din}
Harmonics	A	Fundamental as specified 5 % on the 2 nd harmonic	Fundamental as specified 10 % on the 3 rd harmonic	Fundamental as specified 1 % on the 50 th harmonic	Fundamental as specified Distortion on all harmonics simultaneously up to the 50 th order at 10 % of class 3 compatibility levels from IEC 61000-2-4	Fundamental as specified Distortion on all harmonics simultaneously up to the 50 th order at 200 % of class 3 compatibility levels from IEC 61000-2-4
	S	Fundamental as specified 5 % on the 2 nd harmonic	Fundamental as specified 10 % on the 3 rd harmonic	Fundamental as specified 1 % on the 40 th harmonic	Fundamental as specified Distortion on all harmonics simultaneously up to the 40 th order at 10 % of class 3 compatibility levels from IEC 61000-2-4	Fundamental as specified Distortion on all harmonics simultaneously up to the 40 th order at 100 % of class 3 compatibility levels from IEC 61000-2-4
Interharmonics	A	Fundamental as specified 5 % on the interharmonic at 1,5 × the fundamental frequency	Fundamental as specified 10 % on the interharmonic at 7,5 × the fundamental frequency	Fundamental as specified 1 % on the interharmonic at 49,5 × the fundamental frequency	Fundamental as specified Distortion on 4 selected interharmonics up to the 50 th order at 10 % of class 3 compatibility levels from IEC 61000-2-4	Fundamental as specified Distortion on 4 selected interharmonics up to the 50 th order at 200 % of class 3 compatibility levels from IEC 61000-2-4
	S	N.A.	N.A.	N.A.	N.A.	N.A.

MsV	A	U_{din} applied at the fundamental frequency, with 0 % U_{din} at the Specified carrier frequency	U_{din} applied at the fundamental frequency, with 1 % U_{din} at the specified carrier frequency	U_{din} applied at the fundamental frequency, with 3 % U_{din} at the Specified carrier frequency	U_{din} applied at the fundamental frequency, with 9 % U_{din} at the specified carrier frequency	U_{din} applied at the fundamental frequency, with 15 % U_{din} at the specified Carrier frequency
	S	N.A.	N.A.	N.A.	N.A.	N.A.

Table 2 – List of single "power-system influence quantities"

Power system influence quantities	Class	Testing state S1		Testing state S2	Testing state S3	Testing state S4
Frequency 50 Hz(covers 50 Hz)	A or S	42,5 Hz		50 Hz	57,5 Hz	N.A.
Frequency 60 Hz(covers 60 Hz)	A or S	51 Hz		60 Hz	69Hz	N.A.
Voltage magnitude	A	10% U_{din}		N.A.	200% U_{din}	N.A.
	S	10% U_{din}		N.A.	150% U_{din}	N.A.
Magnitude of current	A or S	10% I_n		N.A.	100% I_n	N.A.
Harmonics (in addition to the specified fundamental signal)	A or S	c% fundamental signal H1: 100% H3: 10% 180° H7: 10% 180° H11: 10% 180° H15: 4% 180° H19: 5% 180° H23: 5% 180	d % fundamental signal H1: 100% H3: 60% 180° H5: 55% 0° H7: 50% 180° H9: 41% 0°	N.A.	N.A.	N.A.
Interharmonics (including ranks below fundamental)	A	N.A.		Frequency = $1,5 \times$ fundamental frequency; 9 % of U_{din}	Frequency = $0,5 \times$ fundamental frequency; 2,5 % of U_{din}	Distortion applied at two interharmonic frequencies simultaneously: 1) Frequency = 2 nd harmonic plus 5 Hz (105 Hz at 50 Hz, and/or 125 Hz at 60 Hz), Magnitude = 4 % of U_{din} 2) Frequency = 2 nd harmonic plus 10 Hz (110 Hz at 50 Hz, and/or 130 Hz at 60 Hz), Magnitude = 6 % of U_{din}

	S	N.A.	Frequency =1,5 × fundamental frequency; 2,5 % of U_{din}	Frequency =0,5 × fundamental frequency; 2,5 % of U_{din}	N.A.
--	---	------	---	---	------
